



RADIOCARBON DATING CERTIFICATE

14 August 2019

Laboratory Code SUERC-87949 (GU52100)
Submitter Rebecca Nicholson
Oxford Archaeology South
Janus House
Osney Mead
Oxford
OX2 0ES
Site Reference BERR18
Context Reference 157
Sample Reference 6
Material charcoal : Prunus sp. roundwood 1 ring
 $\delta^{13}\text{C}$ relative to VPDB -28.7 ‰
Radiocarbon Age BP 2059 \pm 30

N.B. The above ^{14}C age is quoted in conventional years BP (before 1950 AD) and requires calibration to the calendar timescale. The error, expressed at the one sigma level of confidence, includes components from the counting statistics on the sample, modern reference standard and blank and the random machine error.

Samples with a SUERC coding are measured at the Scottish Universities Environmental Research Centre AMS Laboratory and should be quoted as such in any reports within the scientific literature. The laboratory GU coding should also be given in parentheses after the SUERC code.

Detailed descriptions of the methods employed by the SUERC Radiocarbon Laboratory can be found in Dunbar et al. (2016) *Radiocarbon* 58(1) pp.9-23.


For any queries relating to this certificate, the laboratory can be contacted at suerc-c14lab@glasgow.ac.uk.

Conventional age and calibration age ranges calculated by :



Checked and signed off by :



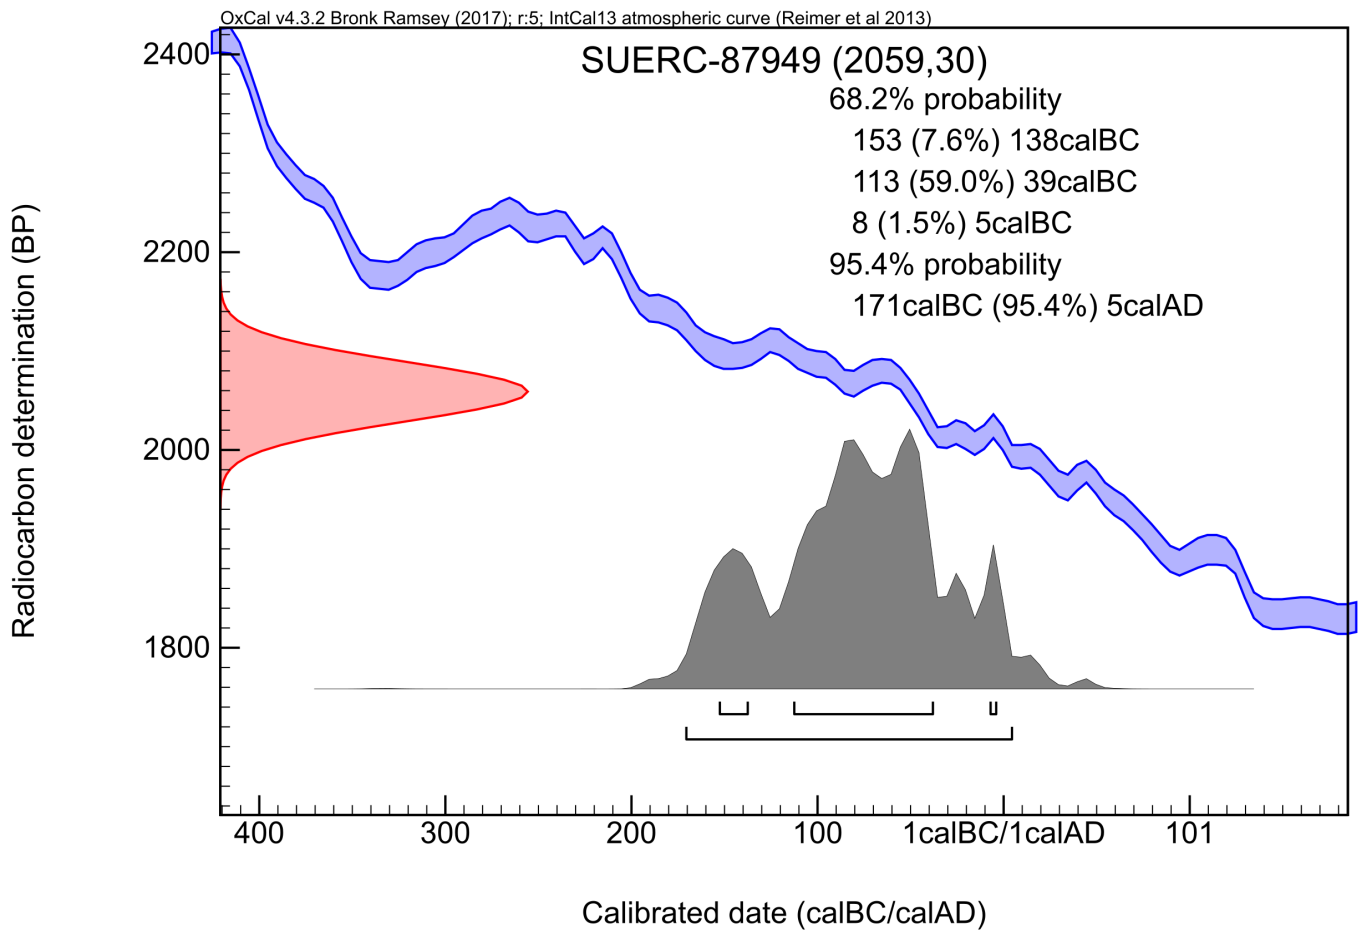

The radiocarbon age given overleaf is calibrated to the calendar timescale using the Oxford Radiocarbon Accelerator Unit calibration program OxCal 4.*

The above date ranges have been calibrated using the IntCal13 atmospheric calibration curve†

Please contact the laboratory if you wish to discuss this further.

* Bronk Ramsey (2009) *Radiocarbon* 51(1) pp.337-60

† Reimer et al. (2013) *Radiocarbon* 55(4) pp.1869-87

RADIOCARBON DATING CERTIFICATE

14 August 2019

Laboratory Code SUERC-87950 (GU52101)

Submitter Rebecca Nicholson
Oxford Archaeology South
Janus House
Osney Mead
Oxford
OX2 0ES

Site Reference BERR18

Context Reference 366

Sample Reference 22

Material charred nut : cf. Prunus sp.

$\delta^{13}\text{C}$ relative to VPDB -26.1 ‰

Radiocarbon Age BP 2471 \pm 30

N.B. The above ^{14}C age is quoted in conventional years BP (before 1950 AD) and requires calibration to the calendar timescale. The error, expressed at the one sigma level of confidence, includes components from the counting statistics on the sample, modern reference standard and blank and the random machine error.

Samples with a SUERC coding are measured at the Scottish Universities Environmental Research Centre AMS Laboratory and should be quoted as such in any reports within the scientific literature. The laboratory GU coding should also be given in parentheses after the SUERC code.

Detailed descriptions of the methods employed by the SUERC Radiocarbon Laboratory can be found in Dunbar et al. (2016) *Radiocarbon* 58(1) pp.9-23.


For any queries relating to this certificate, the laboratory can be contacted at suerc-c14lab@glasgow.ac.uk.

Conventional age and calibration age ranges calculated by :



Checked and signed off by :



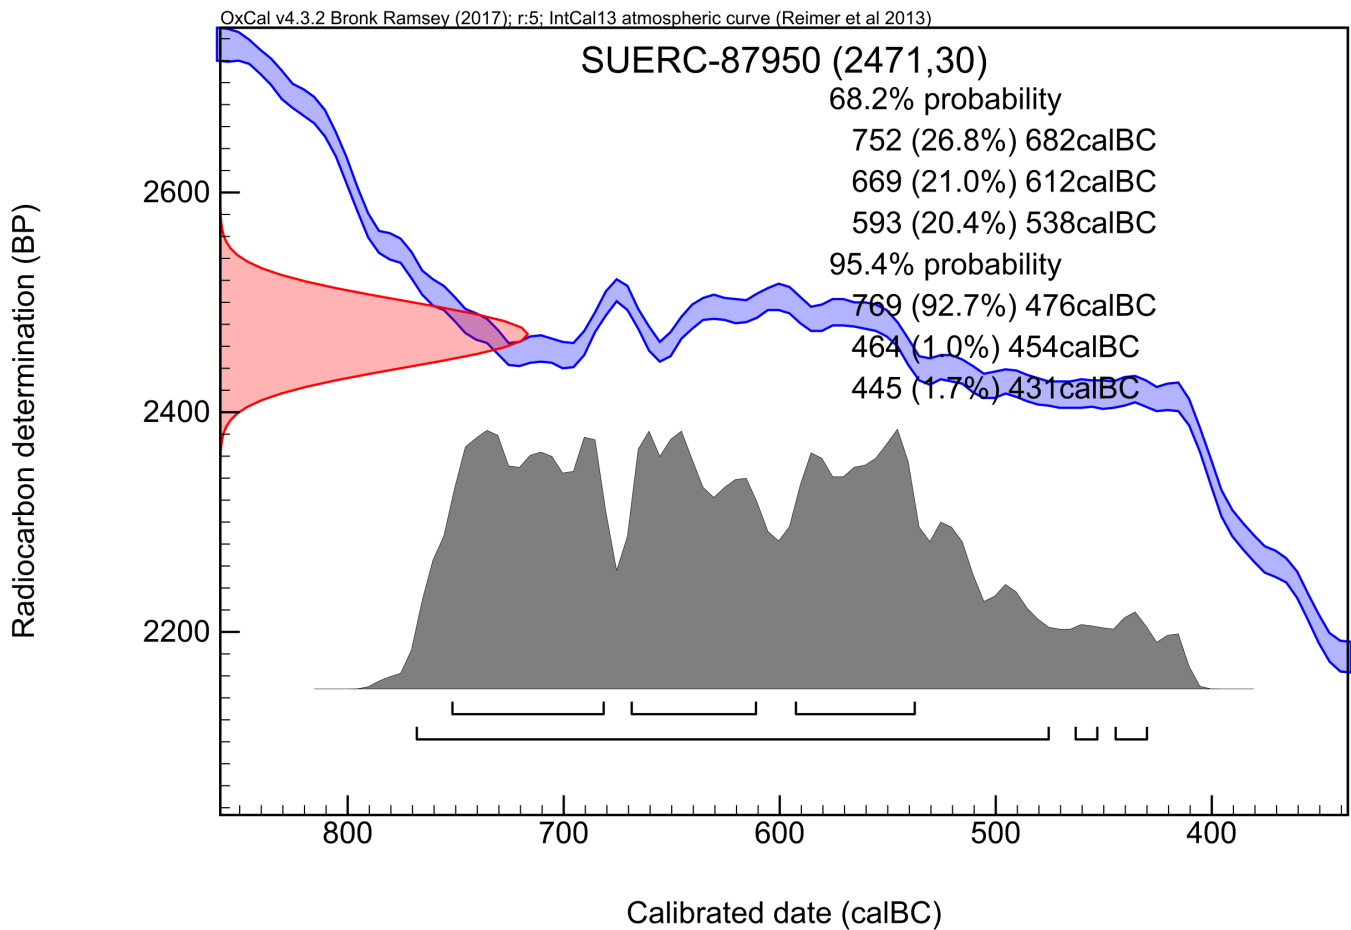

The radiocarbon age given overleaf is calibrated to the calendar timescale using the Oxford Radiocarbon Accelerator Unit calibration program OxCal 4.*

The above date ranges have been calibrated using the IntCal13 atmospheric calibration curve†

Please contact the laboratory if you wish to discuss this further.

* Bronk Ramsey (2009) *Radiocarbon* 51(1) pp.337-60

† Reimer et al. (2013) *Radiocarbon* 55(4) pp.1869-87